
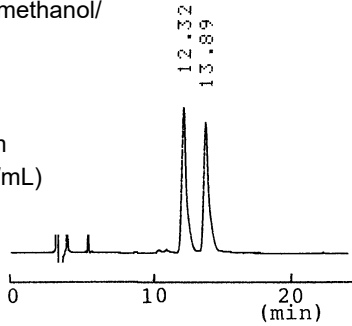
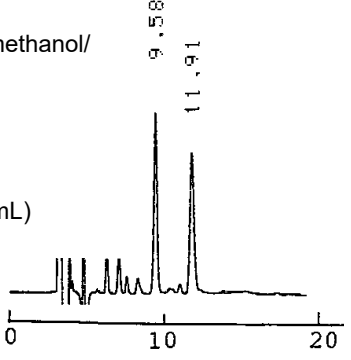
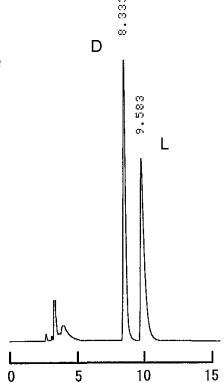
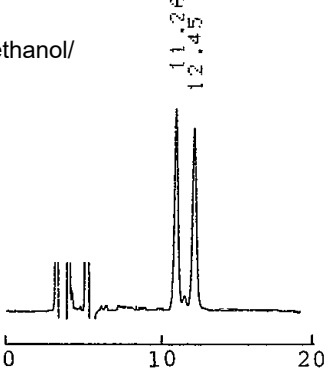
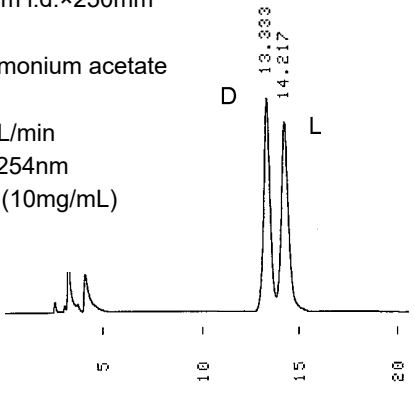
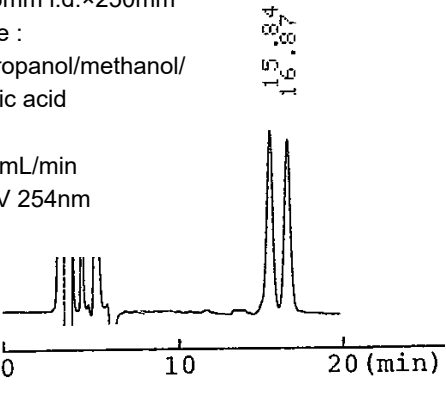



A-34	N-Acetylphenylalanine	
		
<p>OA-4100 $\alpha=1.18$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/2-propanol/methanol/ trifluoroacetic acid (90/5/5/0.2) Flow rate : 1mL/min Detector : UV 254nm Injection : 5µL (5mg/mL)</p> 	<p>OA-4700 $\alpha=1.38$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/2-propanol/methanol/ trifluoroacetic acid (90/5/5/0.2) Flow rate : 1mL/min Detector : UV 254nm Injection : 5µL (5mg/mL)</p> 	
<p>OA-4700 $\alpha=1.24$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : 0.02mol/L ammonium acetate in methanol Flow rate : 1mL/min Detector : UV 254nm Injection : 5µL (10mg/mL)</p> 	<p>OA-4600 $\alpha=1.15$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/2-propanol/methanol/ trifluoroacetic acid (90/5/5/0.2) Flow rate : 1mL/min Detector : UV 254nm</p> 	
<p>OA-4600 $\alpha=1.09$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : 0.02mol/L ammonium acetate in methanol Flow rate : 1mL/min Detector : UV 254nm Injection : 5µL (10mg/mL)</p> 	<p>OA-4500 $\alpha=1.08$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/2-propanol/methanol/ trifluoroacetic acid (90/5/5/0.2) Flow rate : 1mL/min Detector : UV 254nm</p> 	

A-34

N-Acetylphenylalanine

**OA-4000** $\alpha = 1.08$

Column : 4.6mm i.d. x 250mm

Mobile phase :

hexane/2-propanol/methanol/

trifluoroacetic acid

(90/5/5/0.2)

Flow rate : 1mL/min

Detector : UV 254nm

