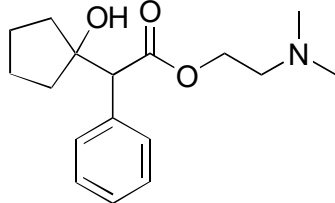
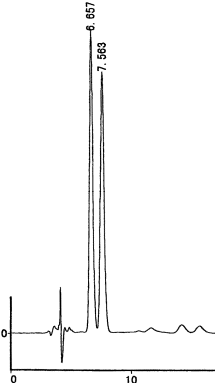
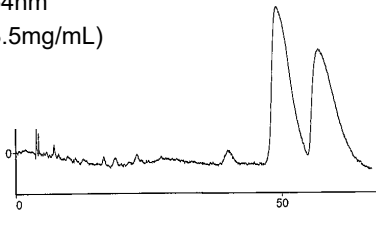

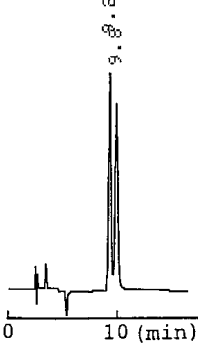
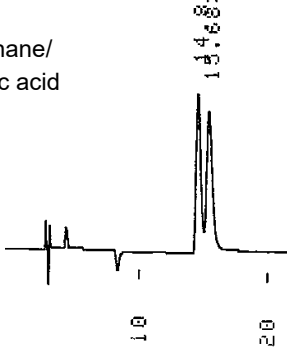
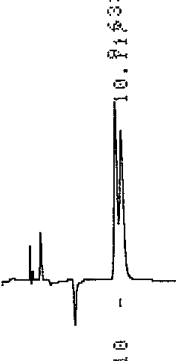
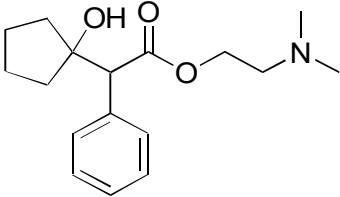
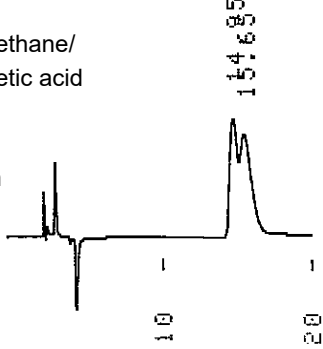


B-11	Cyclopentolate	
		
<p>OA-7000 $\alpha = 1.47$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : acetonitrile/20mmol/L potassium phosphate buffer (pH 3.0) (40/60) Flow rate : 0.7mL/min Detector : UV 254nm Injection : 3µL (3.5mg/mL)</p> 	<p>OA-7100 $\alpha = 1.18$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : acetonitrile/0.1% triethylammonium acetate buffer (pH 5.5) (30/70) Flow rate : 0.7mL/min Detector : UV 254nm Injection : 2µL (3.5mg/mL)</p> 	
<p>OA-4100 $\alpha = 1.09$</p> <p>Column : 4mm i.d.×250mm Mobile phase : hexane/1,2-dichloroethane/methanol/trifluoroacetic acid (250/140/10/1) Flow rate : 1mL/min Detector : UV 254nm</p> 	<p>OA-4700 $\alpha = 1.09$</p> <p>Column : 4mm i.d.×250mm Mobile phase : hexane/1,2-dichloroethane/methanol/trifluoroacetic acid (250/140/10/1) Flow rate : 1mL/min Detector : UV 254nm</p> 	
<p>OA-4400 $\alpha = 1.07$</p> <p>Column : 4mm i.d.×250mm Mobile phase : hexane/1,2-dichloroethane/methanol/trifluoroacetic acid (250/140/10/1) Flow rate : 1mL/min Detector : UV 254nm</p> 	<p>OA-4500 $\alpha = 1.07$</p> <p>Column : 4mm i.d.×250mm Mobile phase : hexane/1,2-dichloroethane/methanol/trifluoroacetic acid (250/140/10/1) Flow rate : 1mL/min Detector : UV 254nm</p> 	

B-11	Cyclopentolate	
		
<p>OA-4800 $\alpha = 1.06$</p> <p>Column : 4mm i.d.×250mm Mobile phase : hexane/1,2-dichloroethane/ methanol/trifluoroacetic acid (250/140/10/1) Flow rate : 1mL/min Detector : UV 254nm</p> 	<p>AGP $\alpha = 1.35$</p> <p>Column : 4mm i.d.×100mm Mobile phase : 1-propanol/10mmol/L sodium phosphate buffer (pH 7.0) (4/96) Flow rate : 0.9mL/min Detector : UV 225nm</p> 