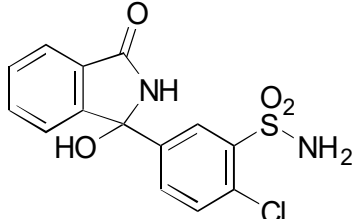
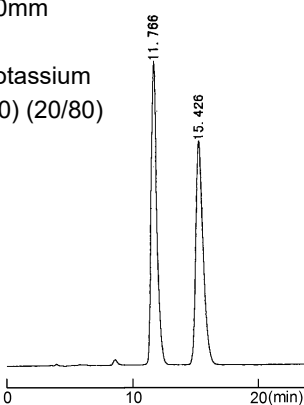
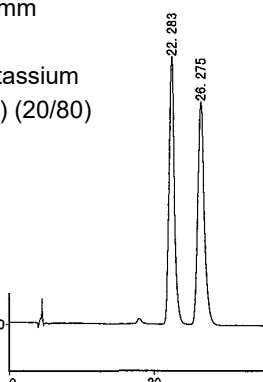
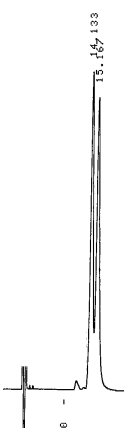
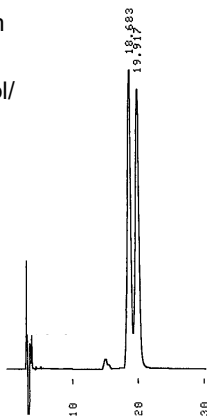
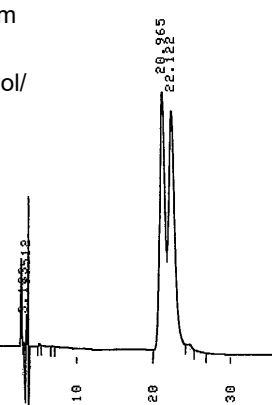


B-32	Chlorthalidone	
		
<p>OA-7000 $\alpha=1.52$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : acetonitrile/20mmol/L potassium phosphate buffer (pH 3.0) (20/80) Flow rate : 0.7mL/min Detector : UV 254nm</p> 	<p>OA-7100 $\alpha=1.23$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : acetonitrile/20mmol/L potassium phosphate buffer (pH 3.0) (20/80) Flow rate : 0.7mL/min Detector : UV 254nm Injection : 5μL (1mg/mL)</p> 	
<p>OA-4600 $\alpha=1.10$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/2-propanol/methanol/trifluoroacetic acid (80/15/5/0.2) Flow rate : 1mL/min Detector : UV 254nm Injection : 5μL (0.7mg/mL)</p> 	<p>OA-4000 $\alpha=1.08$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/2-propanol/methanol/trifluoroacetic acid (80/15/5/0.2) Flow rate : 1mL/min Detector : UV 254nm Injection : 5μL (0.7mg/mL)</p> 	
<p>OA-4400 $\alpha=1.07$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/2-propanol/methanol/trifluoroacetic acid (70/20/10/0.2) Flow rate : 1mL/min Detector : UV 254nm Injection : 5μL (0.7mg/mL)</p> 	<p>AGP $\alpha=2.07$</p> <p>Column : 4mm i.d.×100mm Mobile phase : acetonitrile/10mmol/L sodium phosphate buffer (pH 6.0) (5/95) Flow rate : 0.9mL/min Detector : UV 225nm</p> 