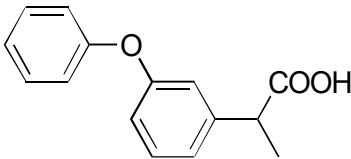
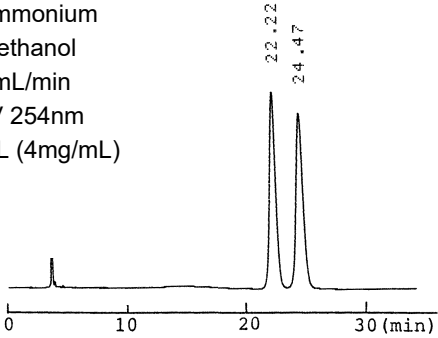
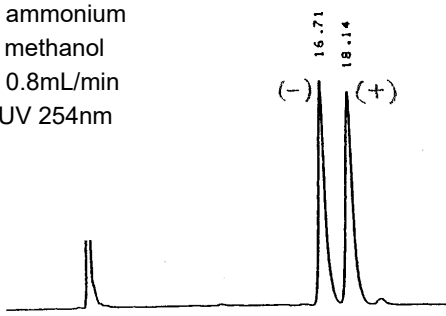



D-01	Fenoprofen	
		
<p>OA-3300 $\alpha = 1.12$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : 0.01mol/L ammonium acetate in methanol Flow rate : 1mL/min Detector : UV 254nm Injection : 2μL (4mg/mL)</p> 	<p>OA-2500 $\alpha = 1.10$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : 0.02mol/L ammonium acetate in methanol Flow rate : 0.8mL/min Detector : UV 254nm</p> 	
<p>AGP $\alpha = 1.28$</p> <p>Column : 4mm i.d.×100mm Mobile phase : 2-propanol/100mmol/L sodium phosphate buffer (pH 7.0) (1/99) Flow rate : 0.9mL/min Detector : UV 225nm</p> 	<p>HSA $\alpha = 1.30$</p> <p>Column : 4mm i.d.×100mm Mobile phase : 10% 2-propanol and 1mmol/L octanoic acid in 10mmol/L sodium phosphate buffer (pH 7.0) Flow rate : 0.9mL/min Detector : UV 225nm</p> 