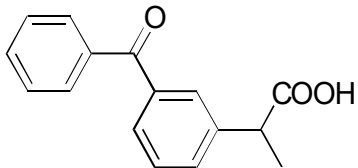


D-02	Ketoprofen	
		
<p>OA-2500 $\alpha=1.18$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : 0.03mol/L ammonium acetate in methanol Flow rate : 1mL/min Detector : UV 254nm Injection : 0.4µL (3.5mg/mL)</p>	<p>OA-3300 $\alpha=1.10$</p> <p>Column : 4mm i.d.×250mm Mobile phase : 0.01mol/L ammonium acetate in methanol Flow rate : 1mL/min Detector : UV 254nm</p>	
<p>AGP $\alpha=2.14$</p> <p>Column : 4mm i.d.×100mm Mobile phase : 1mmol/L dimethyloctylamine in 10mmol/L sodium phosphate buffer (pH 7.0) Flow rate : 0.9mL/min Detector : UV 225nm</p>	<p>HSA $\alpha=1.35$</p> <p>Column : 4mm i.d.×100mm Mobile phase : 10% 2-propanol and 5mmol/L octanoic acid in 10mmol/L sodium phosphate buffer (pH 7.0) Flow rate : 0.9mL/min Detector : UV 225nm</p>	
