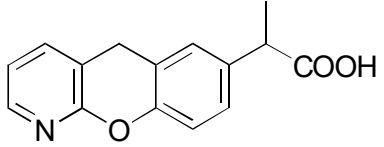
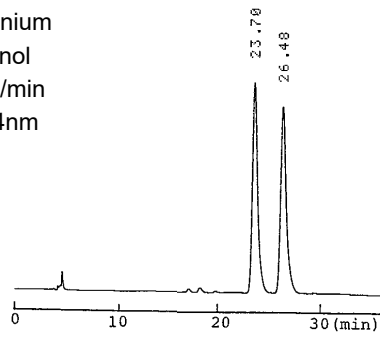
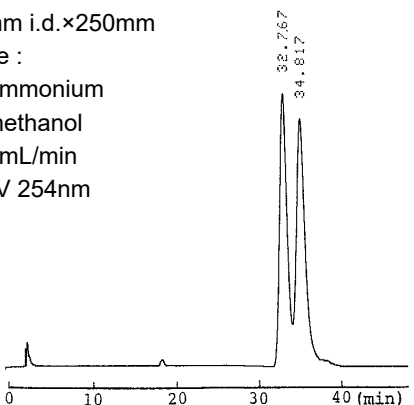


A-07	Pranoprofen		
			
<p><b>OA-2500</b> <math>\alpha=1.13</math></p> <p>Column : 4.6mm i.d.×250mm            Mobile phase :            0.02mol/L ammonium acetate in methanol            Flow rate : 0.8mL/min            Detector : UV 254nm</p> 	<p><b>OA-3200</b> <math>\alpha=1.07</math></p> <p>Column : 4mm i.d.×250mm            Mobile phase :            0.01 mol/L ammonium acetate in methanol            Flow rate : 1mL/min            Detector : UV 254nm</p> 		
<p><b>AGP</b> <math>\alpha=1.15</math></p> <p>Column : 4mm i.d.×100mm            Mobile phase :            acetonitrile/20mmol/L potassium phosphate buffer (pH 3.5) (5/95)            Flow rate : 0.6mL/min            Detector : UV 254nm            Injection : 0.4µL (5mg/mL)</p> 