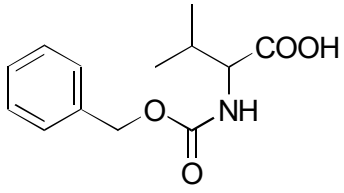
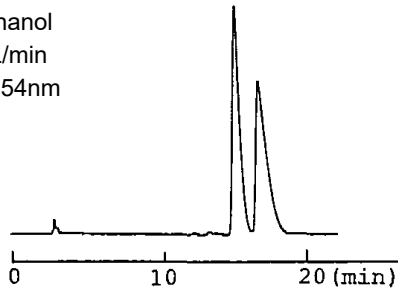
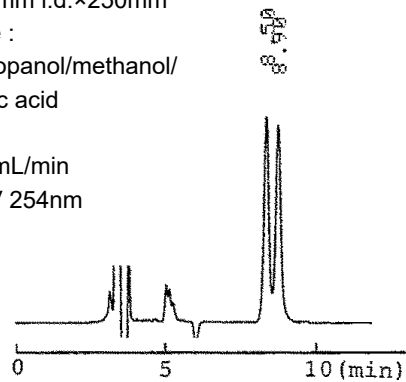
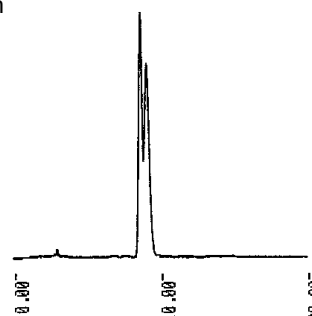
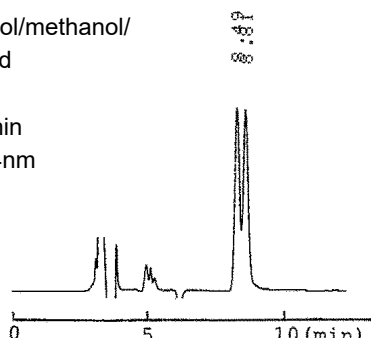


A-09	Z-valine	
		
<p>OA-3200 $\alpha = 1.13$</p> <p>Column : 4mm i.d.×250mm Mobile phase : 0.005mol/L ammonium acetate in methanol Flow rate : 1mL/min Detector : UV 254nm</p> 	<p>OA-4400 $\alpha = 1.08$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/2-propanol/methanol/ trifluoroacetic acid (90/5/5/0.2) Flow rate : 1mL/min Detector : UV 254nm</p> 	
<p>OA-3300 $\alpha = 1.07$</p> <p>Column : 4mm i.d.×250mm Mobile phase : 0.01mol/L ammonium acetate in methanol Flow rate : 1mL/min Detector : UV 254nm</p> 	<p>OA-4500 $\alpha = 1.06$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/2-propanol/methanol/ trifluoroacetic acid (90/5/5/0.2) Flow rate : 1mL/min Detector : UV 254nm</p> 	
<p>OA-4700 $\alpha = 1.06$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : 0.02mol/L ammonium acetate in methanol Flow rate : 1mL/min Detector : UV 254nm Injection : 5µL (6mg/mL)</p> 