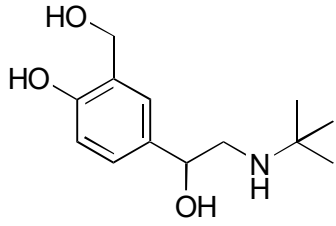
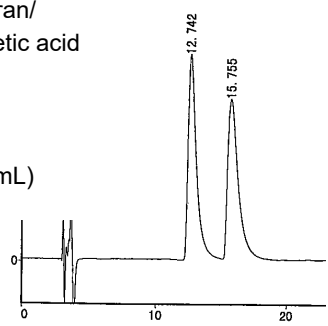
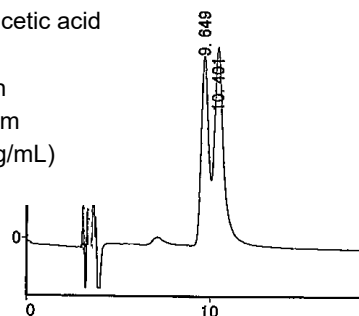


B-03	Salbutamol	
		
<p>OA-4900 $\alpha = 1.32$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/tetrahydrofuran/ methanol/trifluoroacetic acid (60/35/5/0.2) Flow rate : 1mL/min Detector : UV 280nm Injection : 5μL (1mg/mL)</p> 	<p>OA-4700 $\alpha = 1.12$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/tetrahydrofuran/ methanol/trifluoroacetic acid (60/35/5/0.2) Flow rate : 1mL/min Detector : UV 280nm Injection : 5μL (1mg/mL)</p> 	
<p>AGP $\alpha = 1.15$</p> <p>Column : 4mm i.d.×150mm Mobile phase : 10mmol/L sodium phosphate buffer (pH 7.0) Flow rate : 0.9mL/min Detector : UV 225nm</p> 