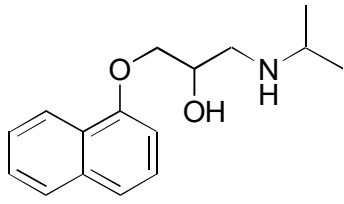
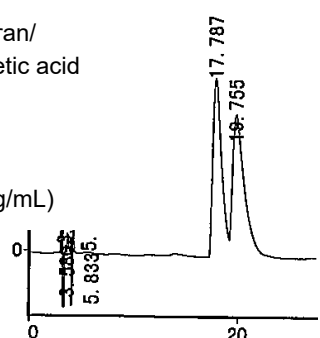
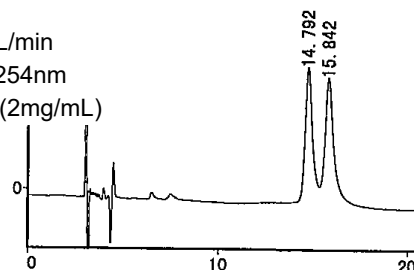


B-01	Propranolol	
		
<p>OA-4900 $\alpha = 1.14$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/tetrahydrofuran/ methanol/trifluoroacetic acid (60/37/3/0.2) Flow rate : 1mL/min Detector : UV 254nm Injection : 2.5µL (2mg/mL)</p> 	<p>OA-4700 $\alpha = 1.09$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : hexane/tetrahydrofuran/ methanol/trifluoroacetic acid (60/38/2/0.2) Flow rate : 1mL/min Detector : UV 254nm Injection : 1µL (2mg/mL)</p> 	
<p>AGP $\alpha = 1.57$</p> <p>Column : 4mm i.d.×100mm Mobile phase : 2-propanol/20mmol/L ammonium acetate buffer (pH 4.1) (0.5/99.5) (total acetate conc.= 110mmol/L) Flow rate : 0.9mL/min Detector : UV 225nm</p> 