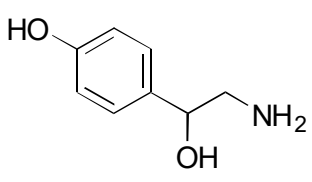


B-16	Octopamine	
		
<p>OA-6000 $\alpha = 1.47$</p> <p>Column : 4.6mm i.d.×150mm Mobile phase : 0.5mmol/L copper(II) sulfate in water Flow rate : 1mL/min Detector : UV 254nm</p>	<p>OA-7700 $\alpha = 1.21$</p> <p>Column : 4.6mm i.d.×250mm Mobile phase : 20mmol/L KH₂PO₄ Flow rate : 0.5mL/min Detector : UV 254nm Injection : 2µL (2mg/mL)</p>	
<p>OA-5000 $\alpha = 1.15$</p> <p>Column : 4.6mm i.d.×150mm Mobile phase : 0.2mmol/L copper(II) acetate and 0.1mol/L ammonium acetate in water (pH 6.5) Flow rate : 1mL/min Detector : UV 280nm</p>	<p>CBH $\alpha = 2.56$</p> <p>Column : 4mm i.d.×100mm Mobile phase : 5% 2-propanol in 10mmol/L sodium phosphate buffer (pH 6.0) + 50 µmol/L EDTA Flow rate : 0.9mL/min Detector : UV 210nm</p>	
