


E-08

Warfarin

**OA-2000** $\alpha=1.22$

Column : 4.6mm i.d.×250mm

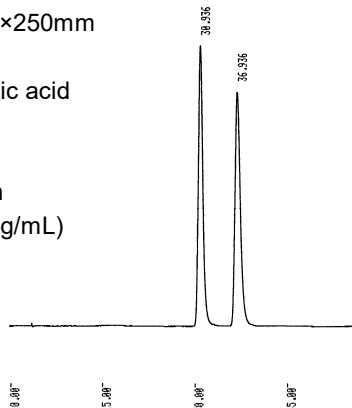
Mobile phase:

hexane/ethanol/acetic acid

(90/10/0.2)

Flow rate : 1mL/min

Detector : UV 254nm

Injection : 5 μ L (2.5mg/mL)**OA-4400** $\alpha=1.10$

Column : 4.6mm i.d.×250mm


Mobile phase:

hexane/ethanol/acetic acid

(90/10/0.2)

Flow rate : 1mL/min

Detector : UV 254nm

**OA-4900** $\alpha=1.11$

Column : 4.6mm i.d.×250mm


Mobile phase:

hexane/ethanol/acetic acid

(90/10/0.2)

Flow rate : 1mL/min

Detector : UV 254nm

Injection : 5 μ L (2.5mg/mL)**AGP** $\alpha=1.42$

Column : 4mm i.d.×100mm

Mobile phase :

2-propanol/10mmol/L sodium phosphate buffer (pH 7.0) (10/90)

Flow rate : 0.9mL/min

Detector : UV 225nm

